

011

Fig. 1

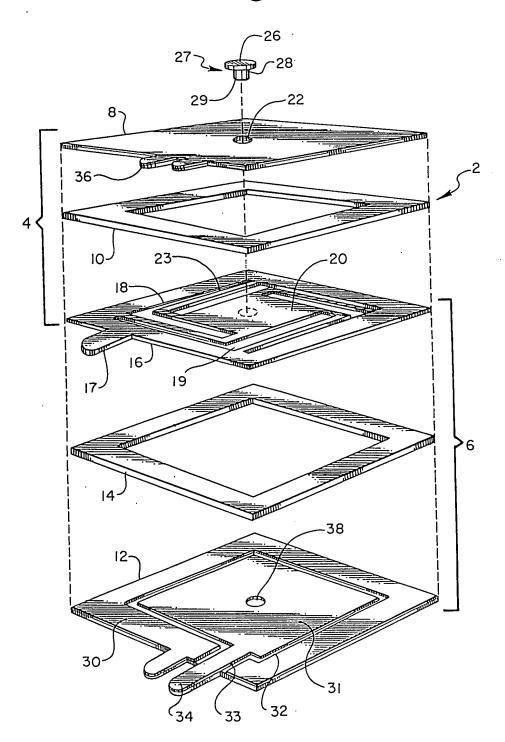

865

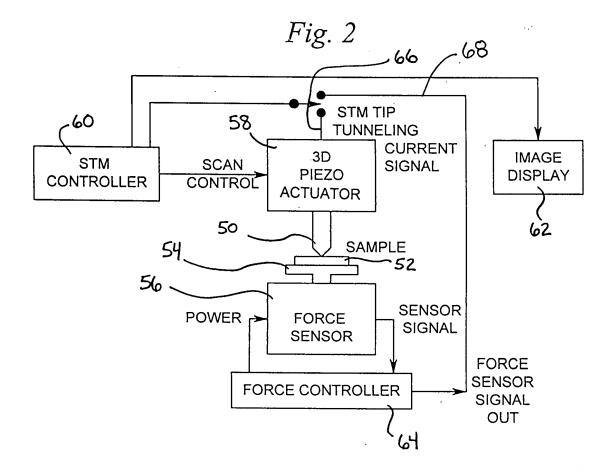

n di e

		100.0 nm		
	2.00			Fig.
		50.0 nm		
	§ -	0.0 nm		
	00.1			
		Microscope Scan size Setpoint Bias Scan rate Number of samples	AS111 STN 2.2 pm 2.2 pm 3.0 pa 3.0 U 2.0 Hz 256	
1.00 2.00	0	Data type Z range	Height 100.0 nm	
	W.			
	•			# 本題

Mig. 4

